


## Acclaim HPLC and UHPLC Columns

### Optimal selectivity through innovative chemistries

Designed for separating a variety of analytes, from small neutral and polar molecules to complex mixtures. Ideal for pharmaceutical, environmental, food and beverage and chemical applications.

- **Diversified Selectivities**  
Novel and proprietary surface chemistries
- **Reproducible and Reliable**  
Strict manufacturing and quality processes
- **High Efficiencies**  
For optimum resolution of complex mixtures
- **Ultra-pure, Porous,  
Spherical Silica**  
Providing consistent quality and performance

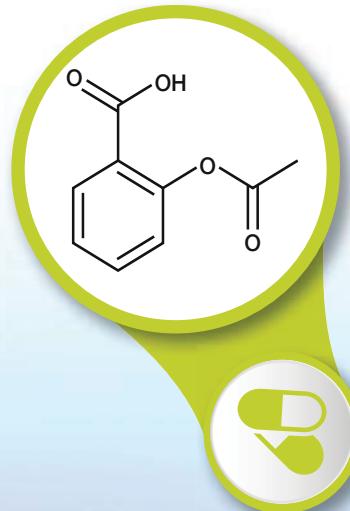


The Acclaim web page contains the latest news, applications and downloads for the Acclaim HPLC column range.  
Visit [www.thermoscientific.com/acclaim](http://www.thermoscientific.com/acclaim)


## Acclaim 120 C18

High performance reversed-phase columns for reproducible results

- High hydrophobic retention
- Excellent efficiencies for maximum resolution
- Low silanol activity for excellent peak shapes for basic analytes
- Extremely low bleed, fully compatible with MS

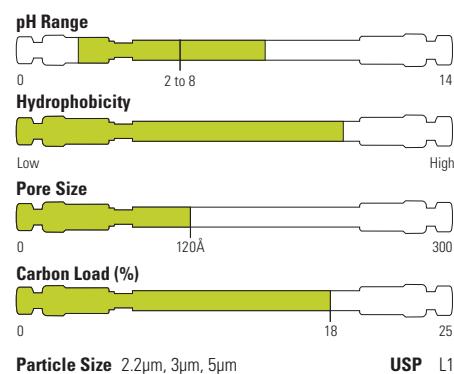

The Acclaim 120 columns are designed for high resolution reversed-phase separations. The very high surface coverage and very low metal content together result in columns with excellent efficiencies. These columns provide exceptional performance for a variety of applications in the pharmaceutical, chemical, environmental and food separations areas.

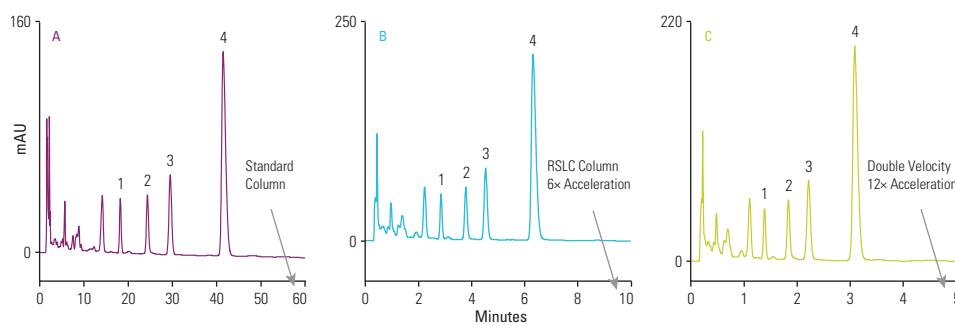

**A: Acclaim 120 C18, 5µm, 150 x 4.6mm  
B, C: Acclaim RSLC C18, 2.2µm, 50 x 2.1mm**

Mobile Phase:	200mM HOAc in 10% (v/v) MeOH
Temperature:	20°C
Flow Rate:	A: 1.00mL/min B: 0.41mL/min C: 0.82mL/min
Injection Volume:	A: 10µL B: 1.2µL C: 1.2µL
Detection:	UV, 254 nm, A: 1 Hz data rate B: 5 Hz data rate C: 10 Hz data rate
Analytes:	1. p-Hydroxybenzoic acid 2. p-Hydroxybenzaldehyde 3. Vanillic acid 4. Vanillin
Sample:	Commercial vanilla extract in 40% ethanol, filtered
Reference:	AOAC Official Method 990.25

### Acclaim 120 C18

Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
2.2	RSLC Column	30	<b>071400</b>	<b>071606</b>	-
		50	<b>068981</b>	<b>071605</b>	-
		75	-	<b>075697</b>	-
		100	<b>068982</b>	<b>071604</b>	-
		150	<b>071399</b>	-	-
		250	<b>074812</b>	-	-
3	HPLC Column	33	-	<b>066272</b>	-
		50	<b>059128</b>	<b>068971</b>	<b>059131</b>
		75	-	<b>066273</b>	-
		100	<b>059129</b>	<b>076186</b>	<b>059132</b>
		150	<b>059130</b>	<b>063691</b>	<b>059133</b>
		250	<b>076187</b>	<b>070077</b>	-
5	Guard Cartridge	10	<b>069689</b>	<b>071981</b>	<b>069695</b>
	HPLC Column	150	-	-	<b>059148</b>
		250	-	-	<b>059149</b>


See page 4-037 for Acclaim Guard Holder Ordering Guide

## Acclaim 120 C8

High performance reversed-phase columns with intermediate hydrophobic retention


- Low silanol activity for excellent peak shapes for basic analytes
- Excellent column efficiencies
- LC-MS compatible

Acclaim 120 C8 reversed-phase columns feature densely bonded monolayer C8 ligands on a high-purity, spherical porous silica substrate. The columns are a well-characterized line of LC-MS compatible C8 phases with very high surface coverage and extremely low silanol activity. These columns provide exceptional performance for a variety of applications in the pharmaceutical, environmental, food and many other industrial sectors.

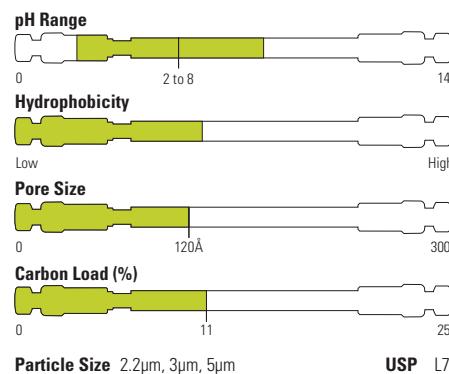

USP L7

### Triclosan in toothpaste

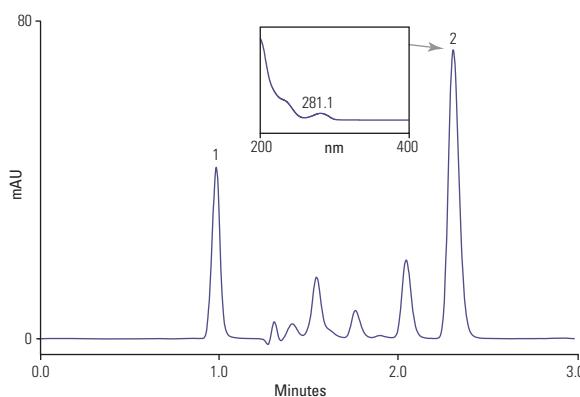

#### Column: Acclaim RSLC C8, 2.2µm, 50 x 2.1mm

Mobile Phase:	Isocratic, 15% buffer, (2mM Ammonium acetate pH5), 85% methanol (v/v)
Temperature:	50°C
Flow Rate:	0.2mL/min
Injection Volume:	1.0µL
Detection:	Diode array detector, 281nm, 10Hz, 0.1 s resp. time and spectra 200–400 nm
Analytes:	1. Saccharin 2. Triclosan
Sample:	Toothpaste containing 0.3% triclosan

### Acclaim 120 C8


Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
2.2	RSLC Column	30	-	<b>072618</b>	-
		50	<b>072615</b>	<b>072619</b>	-
		100	<b>072616</b>	<b>072620</b>	-
		150	<b>072617</b>	-	-
		250	<b>074811</b>	-	-
3	HPLC Column	50	<b>059122</b>	-	<b>059125</b>
		100	<b>059123</b>	-	<b>059126</b>
		150	<b>059124</b>	<b>068970</b>	<b>059127</b>
		250	<b>076185</b>	-	-
5	Guard Cartridge	10	<b>069688</b>	<b>071979</b>	<b>069696</b>
	HPLC Column	50	<b>059134</b>	-	<b>059138</b>
		100	-	-	<b>059139</b>
		150	<b>059136</b>	-	<b>059140</b>
		250	-	-	<b>059141</b>

See page 4-037 for Acclaim Guard Holder Ordering Guide

## Acclaim Phenyl-1

A unique reversed-phase column with high aromatic selectivity


- High aromatic selectivity
- High hydrophobic retention
- Unique and complementary selectivity compared to any other phenyl type column
- Compatibility with highly aqueous mobile phase
- High efficiency and rugged packing

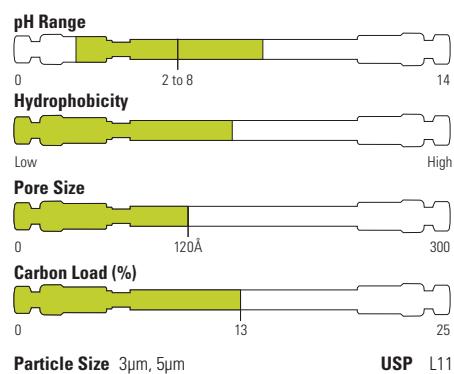

Acclaim Phenyl-1 has a higher pi-pi interaction than other phenyl phases and provides unique selectivity for aromatic compounds while maintaining sufficient hydrophobic interaction and aqueous compatibility for superior chromatographic performance.

The Acclaim Phenyl-1 column can be used in a wide range of applications in pharmaceutical, environmental, food testing and product-quality testing. This column is ideally suited for the analysis of aromatic analytes; some examples include glucocorticosteroids, estrogens, fat-soluble vitamins and phospholipids.

### Separation of fat-soluble vitamins

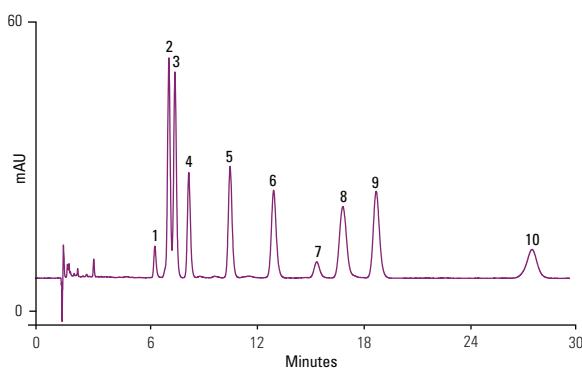

### Acclaim Phenyl-1, 3µm, 150 x 3.0mm

Mobile Phase:	Methanol/water v/v 90/10
Temperature:	30°C
Flow Rate:	0.5mL/min
Injection Volume:	2µL
Detection:	UV, 220nm
Analytes:	(100 ppm each)
	1. Retinol acetate (vitamin A acetate)
	2. Vitamin D2
	3. Vitamin D3
	4. delta-Tocopherol
	5. gamma-Tocopherol
	6. alpha-Tocopherol (vitamin E)
	7. Impurity (unknown)
	8. Vitamin E acetate
	9. Vitamin K2
	10. Vitamin K1

### Acclaim Phenyl-1

Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	Guard Cartridge	10	<b>079934</b>	<b>071974</b>	<b>071973</b>
	HPLC Column	150	<b>071971</b>	<b>071970</b>	<b>071969</b>
5	HPLC Column	150	-	-	<b>088016</b>
		250	-	-	<b>079697</b>

### Acclaim Guard Holder


Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>

## Acclaim C30


Columns for separating structurally related isomers

- High shape selectivity
- Unique selectivity complementary to other reversed-phase columns
- Compatibility with highly aqueous mobile phase
- High-quality: low column bleed, high efficiency and rugged packing

The Acclaim C30 is designed to provide high shape selectivity for separating hydrophobic structural related isomers and unique selectivity complementary to other reversed-phase columns (e.g. C18).

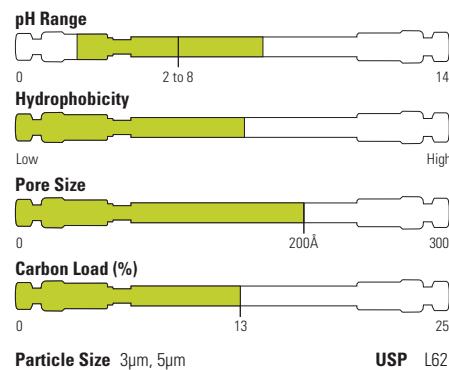

### Omega fatty acids

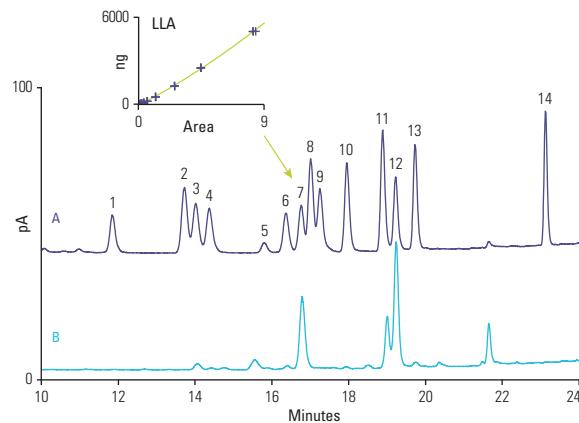

#### Acclaim C30, 5µm, 150 x 4.6mm

Mobile Phase A: Water:formic acid:mobile phase B  
900:3.6:100 (v/v)  
Mobile Phase B: Acetone:acetonitrile:THF:formic acid  
675:225:100:4 (v/v)

Gradient:	Time (min)	%A	%B
0	100	0	
1	40	60	
13	30	70	
22	5	95	
24	5	95	
29	100	0	
32	100	0	

Temperature: 30°C

Flow Rate: 1.00mL/min

Injection Volume: 2µL

Detection: Corona ultra, nebulizer 15°C, filter high

Analytes:

1. SDA
2. EPA
3. ALA
4. GLA
5. DHA
6. Arach.
7. LLA

Samples:

- A. Standards in isopropanol
- B. Saponified chicken fat

### Acclaim C30

Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	HPLC Column	50	<b>078666</b>	-	<b>078661</b>
		100	<b>078665</b>	-	-
		150	<b>075725</b>	<b>075724</b>	<b>075723</b>
		250	<b>078664</b>	<b>075726</b>	-
5	Guard Cartridge	10	<b>075722</b>	<b>075721</b>	<b>075720</b>
	HPLC Column	150	-	-	<b>075719</b>
		250	-	-	<b>075718</b>


### Acclaim Guard Holder

Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>

## Acclaim PolarAdvantage


Novel polar-embedded reversed-phase columns with unique selectivity

- Selectivity complementary to the C18 column
- Low silanol activity for excellent peak shape with basic compounds
- Compatible with 100% aqueous mobile phase
- High selectivity for hydrophobic aromatic molecules
- Wide range of applications

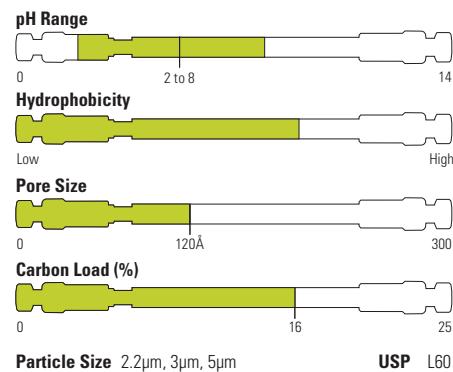

Acclaim PolarAdvantage (PA) columns feature a patented bonding column chemistry that incorporates a polar sulfonamide group with an ether linkage near the silica surface. This unique chemistry provides low silanol activity, compatibility with 100% aqueous mobile phase. The Acclaim PA column offers great separation power to resolve a wide variety of polar and non-polar analytes and supports LC-MS analysis.

### EPA 604 phenols

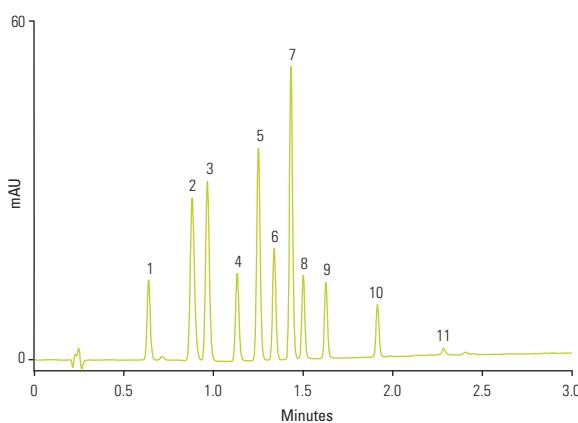

Acclaim RSLC PolarAdvantage, 2.2μm, 50 x 3.0mm											
Mobile Phase A:	10mM formic acid + 10mM ammonium formate, pH 3.75 ± 0.05										
Mobile Phase B:	Acetonitrile										
Gradient:	-1.5 0.0 0.3 2.6 3.0 %A 70 70 70 10 10 %B 30 30 30 90 90										
Temperature:	30°C										
Flow Rate:	1.25mL/min										
Injection Volume:	0.5μL										
Detection:	UV, 280nm, 10Hz, 0.5s resp. time										
Analytes:	1. Phenol 2. 2,4-Dinitrophenol 3. 4-Nitrophenol 4. 2-Chlorophenol 5. 2-Nitrophenol 6. 2,4-Dimethylphenol 7. 4,6-Dinitro-2-methylphenol 8. 4-Chloro-3-methylphenol 9. 2,4-Dichlorophenol 10. 2,4,6-Trichlorophenol 11. Pentachlorophenol										
Sample:	Calibration mix, 50μg/mL in water										


### Acclaim PolarAdvantage

Particle Size (μm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
2.2	RSLC Column	50	<b>072622</b>	-	-
		75	-	<b>075698</b>	-
		100	<b>072623</b>	<b>072627</b>	-
		150	<b>072624</b>	-	-
		250	<b>074813</b>	-	-
3	HPLC Column	50	<b>063174</b>	<b>068972</b>	-
		100	<b>061316</b>	<b>076214</b>	-
		150	<b>061317</b>	<b>063693</b>	<b>061318</b>
		250	-	<b>070079</b>	-
	Guard Cartridge	10	<b>069691</b>	<b>071983</b>	<b>069698</b>
5	HPLC Column	50	-	-	<b>061319</b>
		150	-	-	<b>061320</b>
		250	-	-	<b>061321</b>

## Acclaim PolarAdvantage II

Complementary selectivity and enhanced hydrolytic stability


- Unique selectivity complementary to the C18 column
- Novel polar-embedded column chemistry for hydrolytic stability
- Compatible with 100% aqueous mobile phase
- Low bleed for MS compatibility
- Wide range of applications

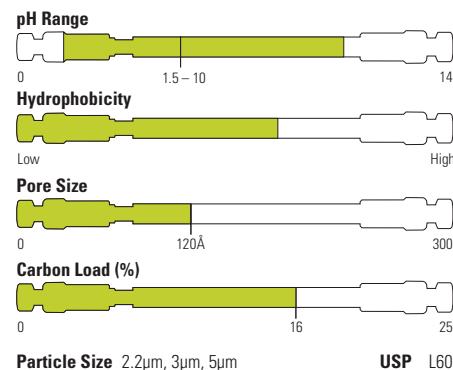

Acclaim PolarAdvantage II (PA2) columns feature a patented surface chemistry that incorporates an amide-embedded polar group and multi-point attachment between the ligands and the silica surface. This unique chemistry provides enhanced hydrolytic stability from pH 1.5-10 with 100% aqueous mobile phases and exhibits high reversed-phase capacity, with selectivity complementary to conventional C18 columns.

The Acclaim PA2 column is specifically designed to withstand high pH conditions, making it a good choice for the separation of both basic and acidic analytes.

### Turmeric

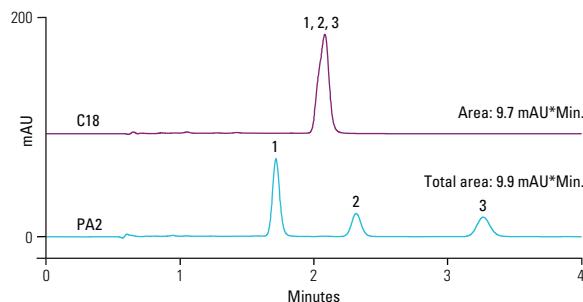

#### Acclaim RSLC 120 C18 2.2μm, 100 x 2.1mm Acclaim RSLC PA2, 2.2μm, 100 x 2.1mm

Mobile Phase A: 15mM H<sub>3</sub>PO<sub>4</sub>  
 Mobile Phase B: Methanol  
 Isocratic: C18: 70% B (v/v)  
 PA2: 80% B (v/v)  
 Temperature: 30°C  
 Flow Rate: 0.41mL/min  
 Detection: UV, 428nm  
 Analytes: 1. Curcumin  
 2. Demethoxycurcumin  
 3. Bis-demethoxycurcumin  
 Sample: Turmeric extract

### Acclaim PolarAdvantage II


Particle Size (μm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
2.2	RSLC Column	30	<b>071402</b>	<b>071609</b>	-
		50	<b>068989</b>	<b>071608</b>	-
		100	<b>068990</b>	<b>071607</b>	-
		150	<b>071401</b>	-	-
		250	<b>074814</b>	-	-
3	HPLC Column	33	-	<b>066276</b>	-
		50	<b>077999</b>	<b>068973</b>	<b>063189</b>
		75	-	<b>066277</b>	-
		100	<b>077998</b>	<b>078000</b>	<b>078001</b>
		150	<b>063187</b>	<b>063705</b>	<b>063191</b>
		250	<b>077997</b>	<b>070080</b>	-
5	Guard Cartridge	10	<b>069692</b>	<b>071985</b>	<b>069699</b>
	HPLC Column	150	-	-	<b>063197</b>
		250	-	-	<b>063199</b>

See page 4-037 for Acclaim Guard Holder Ordering Guide

## Acclaim HILIC-10


Designed with unique selectivity for hydrophilic molecules

- Retains highly polar molecules that are not retained by reversed-phase chromatography
- Unique selectivity, complementary to reversed-phase columns
- Hydrolytically stable
- Rugged column packing
- Broad application range

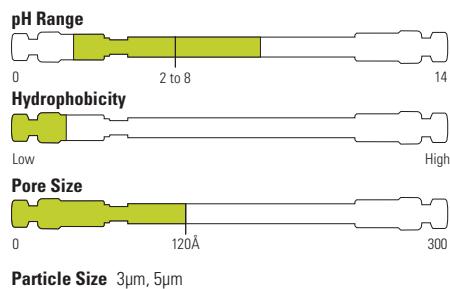

The Acclaim HILIC-10 column is designed for separating highly hydrophilic molecules by Hydrophilic Interaction Liquid Chromatography (HILIC). This column is based on high-purity spherical porous silica covalently modified with a proprietary hydrophilic layer.

### Glycerides

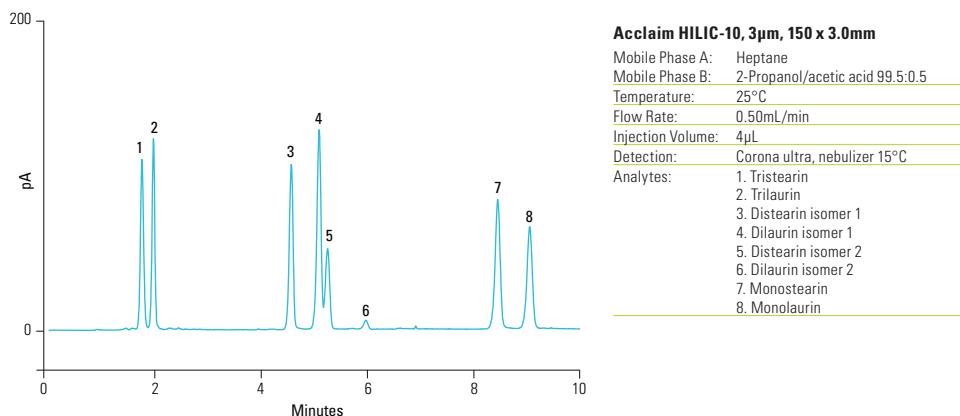

### Acclaim HILIC-10

Particle Size (μm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	HPLC Column	150	<b>074259</b>	<b>074258</b>	<b>074257</b>
5	Guard Cartridge	10	<b>074263</b>	<b>074261</b>	<b>074262</b>


### Acclaim Guard Holder

Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>

## Acclaim Mixed-Mode HILIC-1

Uniquely designed for both reversed-phase and HILIC operations


- Can operate in both RP and HILIC modes
- Retains highly polar molecules
- Unique selectivity complementary to RP columns
- Broader application range compared with conventional diol-based columns
- High-efficiency column for high-resolution separations

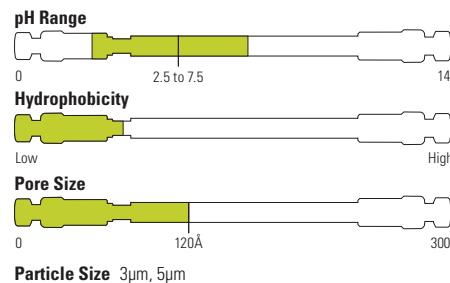

The Acclaim Mixed-Mode HILIC-1 column features a unique, high-efficiency, silica-based HPLC mixed-mode stationary phase that combines both reversed-phase (RP) and hydrophilic interaction liquid chromatography (HILIC) properties. This combination allows both hydrophobic and hydrophilic interactions to be utilized to optimize separations.

The functional group is of a hydrophobic alkyl chain with a diol group at the terminus. This unique combination results in the adjustable selectivity, making Acclaim Mixed-Mode HILIC-1 separate mixtures that would be impossible for a C18 column. This column is suitable for a broad range of applications, including non-ionic ethoxylated surfactants, drug metabolites, lipids, polyethylene glycols (PEGs), ethoxylated surfactants, and more.

### Cytosine and naphthalene

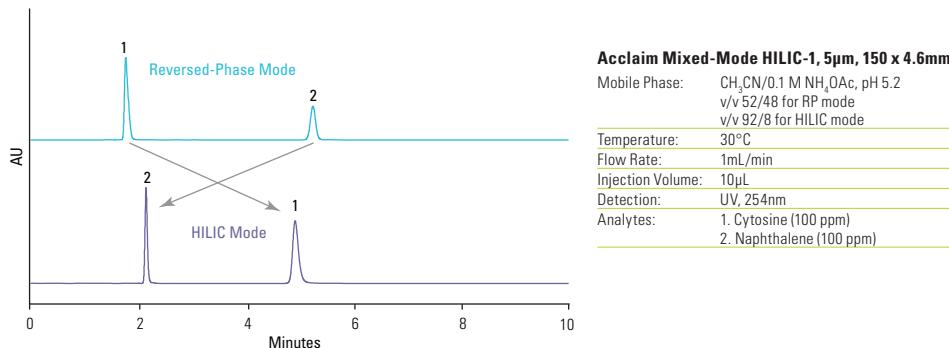

### Acclaim Mixed-Mode HILIC-1

Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	HPLC Column	50	-	<b>071912</b>	-
		150	<b>070091</b>	<b>070090</b>	-
5	Guard Cartridge	10	<b>069694</b>	<b>071913</b>	<b>069706</b>
		150	<b>066847</b>	-	<b>066843</b>
	HPLC Column	250	-	-	<b>066844</b>

### Acclaim Guard Holder

Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>


## Acclaim Mixed-Mode WAX-1

Designed for separating anionic molecules with powerful adjustable selectivity control

- Adjustable selectivity
- Selectivity orthogonal to reversed-phase (RP) columns
- Ideal selectivity for anionic molecules
- Excellent column efficiency and peak asymmetry
- Multimode retention mechanisms: reversed-phase, weak anion exchange, and HILIC modes

The Acclaim Mixed-Mode WAX-1 is a novel, high-efficiency silica HPLC column that combines hydrophobic and weak anion exchange characteristics. Its unique chemistry results in a multimode separation mechanism that includes reversed-phase, anion exchange, and HILIC interactions. Selectivity can be adjusted by changing ionic strength, pH or organic solvent content.

### Pain relief medicine

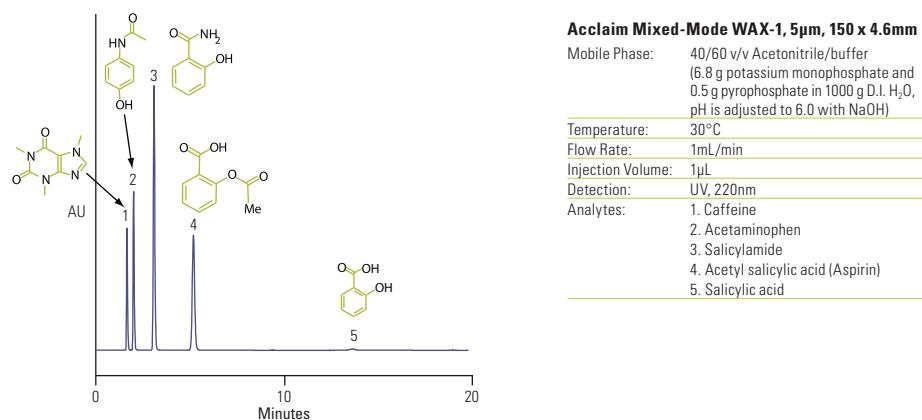


### Acclaim Mixed-Mode WAX-1

Particle Size (µm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	HPLC Column	50	-	<b>071908</b>	-
		150	<b>070089</b>	<b>070088</b>	-
5	Guard Cartridge	10	<b>069686</b>	<b>071909</b>	<b>069704</b>
		150	<b>067084</b>	-	<b>064984</b>
	HPLC Column	250	-	-	<b>064985</b>

### Acclaim Guard Holder

Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>

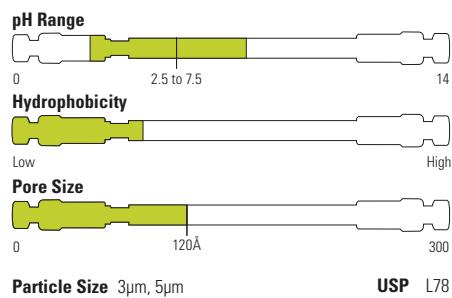


## Acclaim Mixed-Mode WCX-1

Designed for separating cationic molecules with adjustable selectivity control


- Adjustable selectivity
- Ideal selectivity for separating basic molecules
- Selectivity complementary to C18 RP columns
- Multimode separation mechanism: reversed-phase, weak cation exchange, anion-exclusion and HILIC

The Acclaim Mixed-Mode WCX-1 is a novel, high-efficiency, silica-based column, with a proprietary ligand with both hydrophobic and weak cation exchange properties. Selectivity of ionizable and neutral compounds can be controlled independently or simultaneously by tuning mobile phase ionic strength, pH or organic modifier. This column therefore can separate using multiple separation modes: reversed-phase, cation exchange, and normal-phase/ HILIC and is recommended for a variety of industrial applications, including pharmaceutical, chemical, consumer products, foods and beverages.

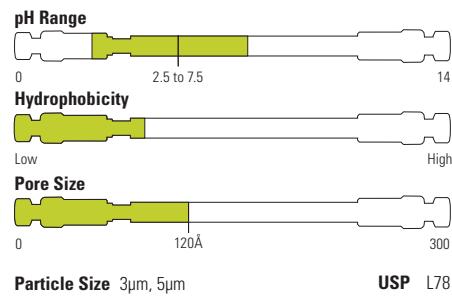

USP L78

### Pharmaceutical counterions

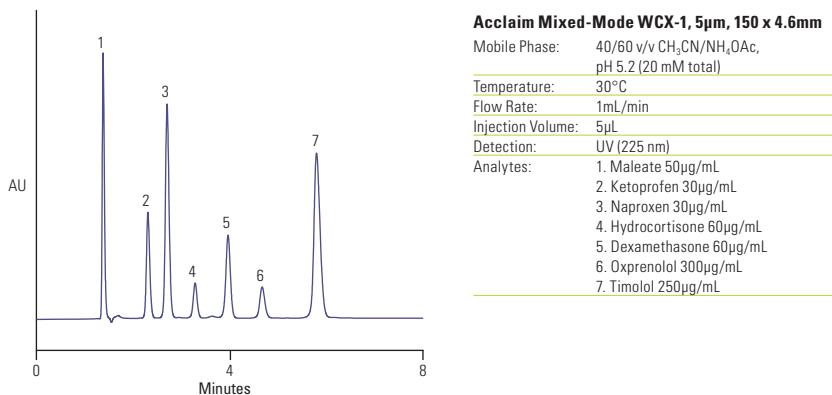

### Acclaim Mixed-Mode WCX-1

Particle Size (μm)	Format	Length (mm)	2.1mm ID	3.0mm ID	4.6mm ID
3	HPLC Column	50	-	<b>071910</b>	-
		150	<b>070093</b>	<b>070092</b>	-
5	Guard Cartridge	10	<b>085455</b>	<b>071911</b>	<b>069705</b>
		150	<b>068371</b>	-	<b>068353</b>
	HPLC Column	250	-	-	<b>068352</b>

### Acclaim Guard Holder

Format	Cat. No.
Acclaim Guard Cartridge Holder V-2	<b>069580</b>
Acclaim Guard Kit (Holder and Coupler) V-2	<b>069707</b>
Guard to Analytical Column Coupler V-2	<b>074188</b>

## OmniPac


DVB polymer columns for combined ion exchange and reversed-phase separations



- Acid, base and solvent compatible, pH 0 to 14
- Ideal for the separation of high molecular weight organic acids
- Delivers optimal separation of very hydrophobic anions
- Delivers optimal separation of halogenated anions
- Provides simultaneous separation of neutral and ionic species
- Unique selectivity for polar and ionic organic analytes
- Delivers optimal separation of organic, hydrophobic, and halogenated cations

Thermo Scientific™ OmniPac™ is a range of latex-based columns. Both PAX columns have an ion exchange capacity of about 40μeq per column, and the PCX columns have a capacity of approximately 120μeq per column. The PAX-500 and PCX-500 columns separate analytes through both ion exchange and reversed-phase mechanisms, due to their higher reversed-phase capacity relative to the PAX-100 and PCX-100 columns.

### Gradient separation of nitrogen-containing compounds

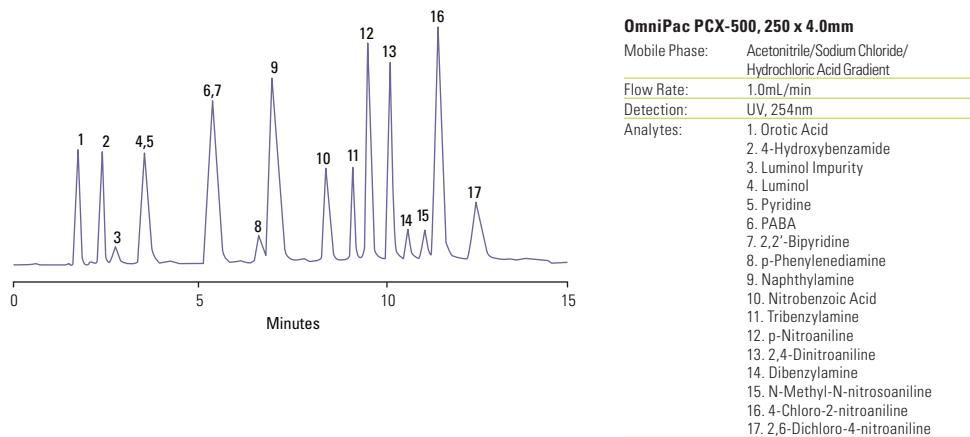

### OmniPac Anion Exchange

Description	Porosity	Length (mm)	4.0mm ID
PAX-100	Microporous	50	<b>042151</b>
		250	<b>042150</b>
PAX-500	Microporous	50	<b>042153</b>
		250	<b>042152</b>

### OmniPac Cation Exchange



Description	Porosity	Length (mm)	4.0mm ID
PCX-100	Microporous	50	<b>042193</b>
		250	<b>042189</b>
PCX-500	Microporous	50	<b>042195</b>
		250	<b>042191</b>

## Acclaim Size Exclusion Chromatography (SEC)


High performance SEC columns for analysis of water soluble polymers

- Proprietary mono-dispersed multi-pore hydrophilic resin: no inflection points in calibration curve
- SEC-300 calibrated from 100 to 50,000 Daltons
- SEC-1000 calibrated from 1,000 to 1,000,000 Daltons
- Availability of small particle sizes packed in 300 x 4.6mm dimension allows for high-resolution analysis at reduced solvent consumption
- Stable surface bonding with low column bleed and compatibility with UV, RI, MS, ELSD and Thermo Scientific™ Dionex™ Corona™ Charged Aerosol Detectors

Thermo Scientific™ Acclaim™ SEC-300 and SEC-1000 are a family of resin based, high performance size exclusion chromatography columns specifically designed for the separation of water soluble polymers and oligomers.

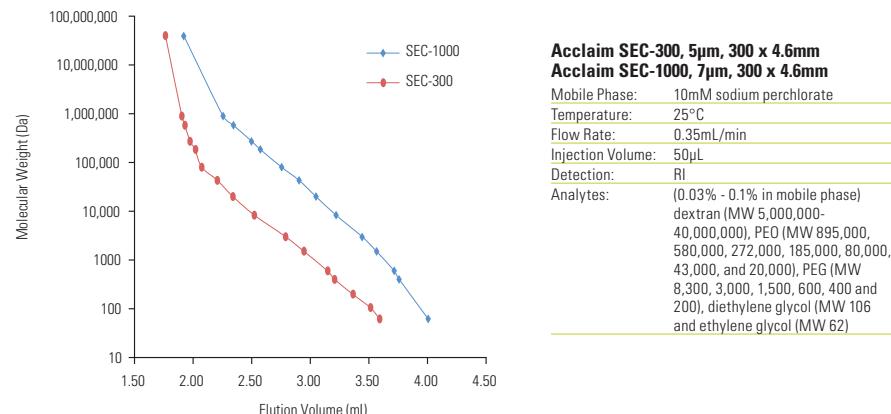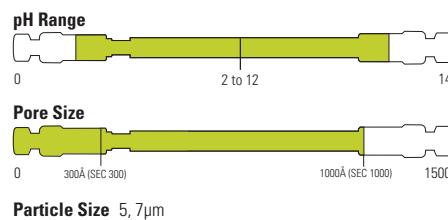

### Polyacrylic acid using size-exclusion chromatography with charged-aerosol detection

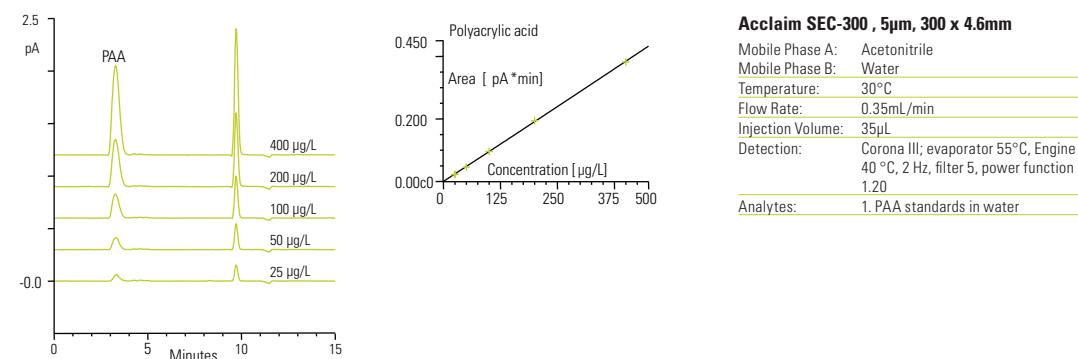

### Acclaim Size Exclusion Chromatography (SEC)

Description	Particle Size (µm)	Format	Length (mm)	4.6mm ID	7.8mm ID
Acclaim SEC-300	5	Guard	33	<b>082740</b>	—
		HPLC Column	150	—	<b>079726</b>
			300	<b>079723</b>	<b>079725</b>
Acclaim SEC-1000	7	Guard	33	<b>082739</b>	—
		HPLC Column	150	—	<b>079722</b>
			300	<b>079724</b>	<b>079721</b>